

Category : **Sepsis/septic shock: management**

A274 - Hemoperfusion with the efferon ct extracorporeal adsorbers containing mesoporous styrene-divinylbenzene copolymer (sdc) in patients with severe covid-19

M Magomedov¹; T Kim¹; S Masolitin¹; A Yaralian¹; E Kalinin¹; V Pisarev²

¹*Pirogov City Clinical Hospital No. 1, Moscow, Russian Federation*, ²*Federal Research and Clinical Center of Intensive Care medicine and Rehabilitology, V.A.Negovsky Institute of General Reanimatology, Moscow, Russian Federation*

Introduction:

Direct extracorporeal removal of inflammatory mediators with various adsorbents has been suggested as a novel treatment modality for COVID-19 patients [1]. Our study determined safety, feasibility and effectiveness of clinical use of a hemoperfusion (HP) with a novel SDC adsorbents to remove pro-inflammatory molecules from the bloodstream of COVID-19 patients.

Methods:

42 COVID-19, PCR+ patients, age <81 years, average 63 (SD range, 54-69) years, 52% men, lethality 48%, underwent standard treatment for COVID-19. On day 0 patients exhibited (median and IQR): PaO₂/FiO₂ 160 (130-200); APACHE II 18 (18-20); SOFA 6.5 (6-8); IL-6 841(709-1424) pg/ml, CRP 109 (84-140) mg/l; ferritin 628 (547-678) µg/L. Group 1 (n=29) continued to receive standard treatment whereas group 2 (n=13) received HP procedure once, for 3-4 hrs, using Efferon CT adsorbents containing mesoporous SDC beads uptaking 6-60 kD molecules [2, 3] followed by continuous veno-venous hemodiafiltration. Groups matched on age and sex; group 2 included more severe patients requiring HP support. Data were treated using R-statistics by XLStat.

Results:

Despite significant intergroup differences in disease severity as shown by SOFA, ALT, AST, SpO₂, pH, lactate, LDH, and IL-6 alterations on day 0, the HP treatment resulted in no difference in lethality between groups. Patients on HP experienced pH increase and rapid decline of SOFA and lactate as covariates most contributed to lethal outcome; IL-6 and ferritin levels significantly decreased vs. group 1 (Figure 1). Decreased lethality by HP was significant in a subset of patients on mechanical ventilation exhibiting SOFA <9 (P=0.024 vs. group 1).

Conclusion:

Anti-cytokine HP with Efferon CT adsorbents is feasible and safe method providing a lifesaving promise for a subset of patients with COVID-19 that warrants extended clinical trials.

References:

1. Ronco C. et al. *Blood Purif.* 50(1):17-27, 2021. 2. Tsyurupa M.P., Davankov V.A. 53 (2-3):193-203, 2002. 3. Bessonov I.V. et al. *WO 2018/217137 A1*, 2018.

Image :

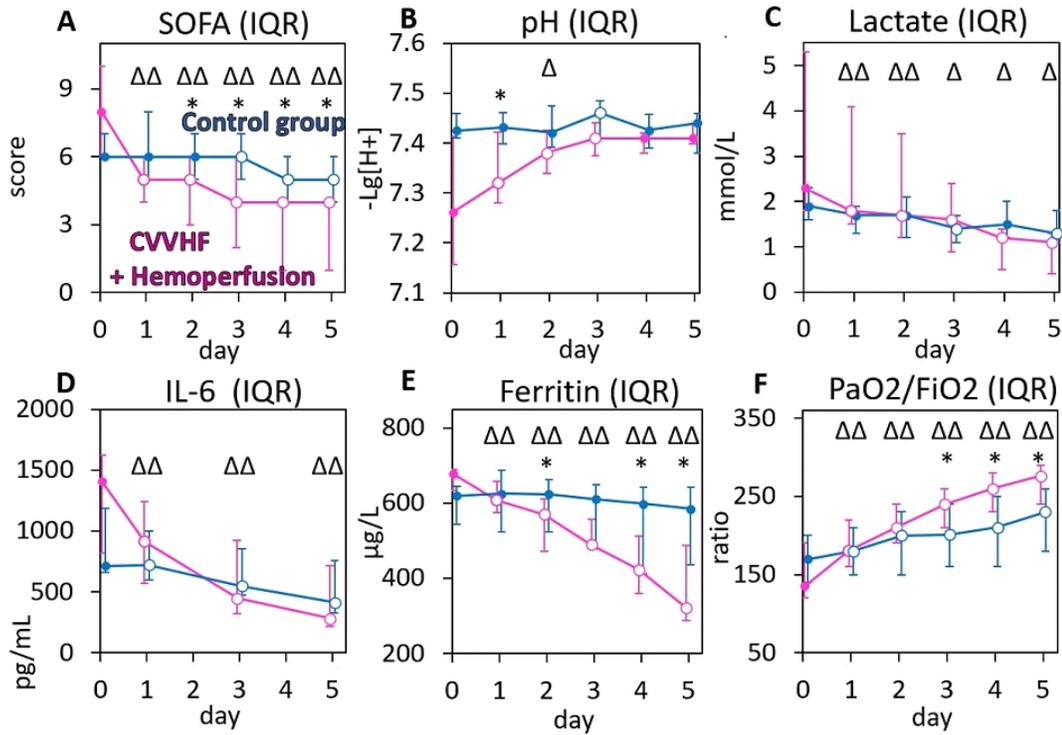


Figure 1. Dynamics of covariates following hemoperfusion (HP) with Efferon CT of severe COVID-19 patients. A-C: covariates contributed most (>30%, $P < 0.005$) to lethality in the cohort ($n=42$), logistic regression model. D-E: other clinically significant covariates recovered following HP. * - $p < 0.05$, Mann-Whitney U test, HP (pink line) vs. no HP (blue line). Δ - $p < 0.05$, $\Delta\Delta$ - $p < 0.001$, Mann-Whitney U test for relative changes (from day 0 to day N) of variables, HP (pink line) vs. no HP (blue line).